



**ICAR- NATIONAL RESEARCH CENTRE ON PIG
INDIAN COUNCIL OF AGRICULTURAL RESEARCH
RANI, GUWAHATI-781131(ASSAM)
Phone/Fax-0361-2847195/2847946**



File No .177/NRCP/2017-18

Date: 28.02.2018

Sub: E-TENDER ENQUIRY FOR Modular Lab Furniture and Fittings...reg.

The Director, ICAR-NRC on Pig, Rani, Guwahati invites e-Tender for Modular Lab Furniture and Fitting at ICAR-NRC on Pig, Guwahati under following terms & conditions:

Closing Date of submission of online Tenders in CPP Portal: 21.03.2018 at 1.00 PM

Opening Date of Online Tenders: 22.03.2018 at 1.00 PM onwards.

TECHNICAL SPECIFICATIONS

One unit of fixture will consist of lab work bench and working table.

Total quantity required- TWO UNITS.

Specifications

General:

The entire unit should have elegant wood finish. High quality thick pre-laminated particle board (PLPB) or chemical resistant material conforming to relevant BIS Specifications such as 12823 – 1990 (EXT) should only be used. Chemically treated board should not warp, bulge, shrink, be brittle and develop cracks. CRCA sheet, if used should be of non-ageing quality, conforming to IS 513: 2008 and amendments. The entire unit should be aesthetically designed with long term durability.

a. LAB WORK BENCH (One on both sides)

The unit will stand on metal with C or similar frames on with pre laminated high quality particle board or similar material. All exposed edges should be smoothed with edge banding. The unit will have four leg spaces (two inside each lab top and working table). The unit will be supplied in modular pattern for rearrangement. Each unit will be provided with one side drawer consisting of one small drawer and one box drawer unit with locking facility.

FINISH: All the metal part will be powder coated to thickness not less than 60 micron in desired shade/colour.

WORKTOP: Worktop should be made of black coloured high quality granite of minimum thickness 18mm along with accessories and fitting resistant to acid, alkali and heat treatments. The granite top should have rounded edges on all exposing sides to avoid physical injury.

REAGENT RACK: Each Work Bench will be consist of one Reagent Rack made of minimum 25mm thick PLPB movable on the top of the work bench.

DIMENSION OF REAGENT RACK : 1000mmW x 300mm D x 700mm H (approximate)

PEDESTAL UNIT: The unit will consist of 2 Nos. Pedestal units made up 1.2mm thick CRCA sheet consisting of 1 No. drawer unit & 1 No. box unit.

ELECTRICAL POINTS: Each Work Bench should be provided with a minimum of 02 Nos. Power point with 16/5 Amp. Modular switch and Socket Points and each Reagent Rack will have a minimum of 02 Nos. power points with 16/5 Amp. All the electrical points should be modular

b. WORKING TABLES (One on both sides)- please see the diagram. All the working table will have wooden finish and chosen colour.

The unit will stand on a minimum of 18mm thick or better pre-laminated particle board (PLPB) or other chemical resistant material confirming to relevant BIS Specifications with height adjuster. All exposed edges should be provided with PVC edge banding pasted with hot melt glue, adjacent to the granite top table.


WORKTOP: Worktop will be 25mm thick pre-laminated particle board (PLPB) or chemical resistant material confirming to relevant BIS Specifications of chosen colour. All exposed edges should be PVC edge banded of thickness 1 mm.

Two spot lights/side have to be fixed over the reagent racks on each and one spot light inside the working tables.


High quality laboratory working stools (4 nos) and revolving chairs with back rest (4 nos) with soft cushion to be supplied.

All dimensions are approximate (indicated in the figures) and may be suitably modified to improve utility, aesthetic look, stability and durability of the structure.


The furniture and fixture should have a warranty of 5 years or more.

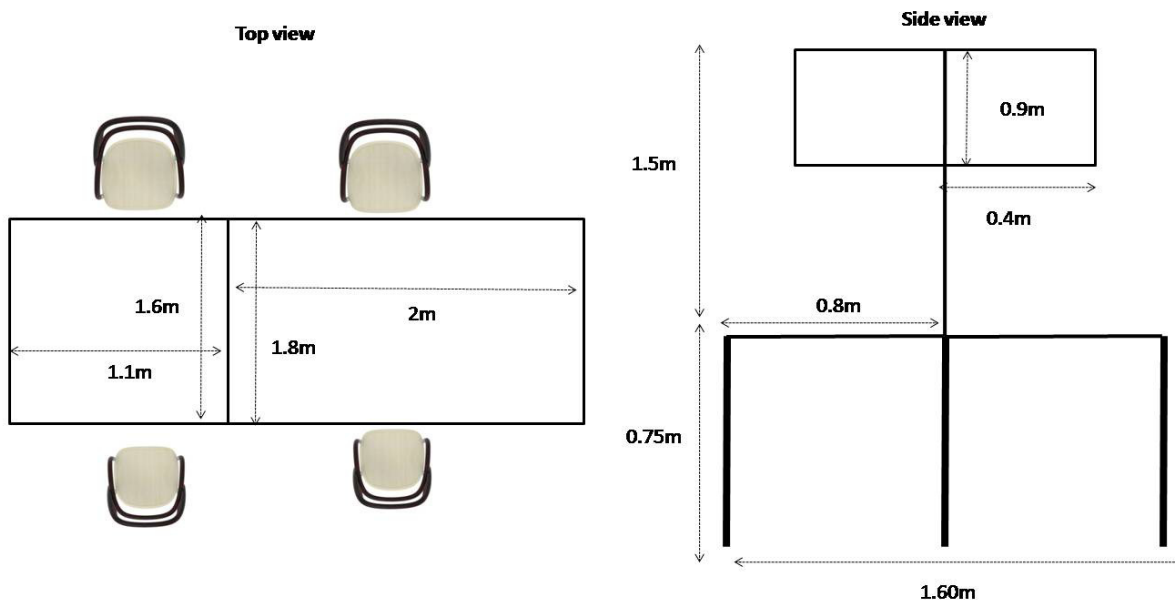

Proposed outlay of units in the laboratory

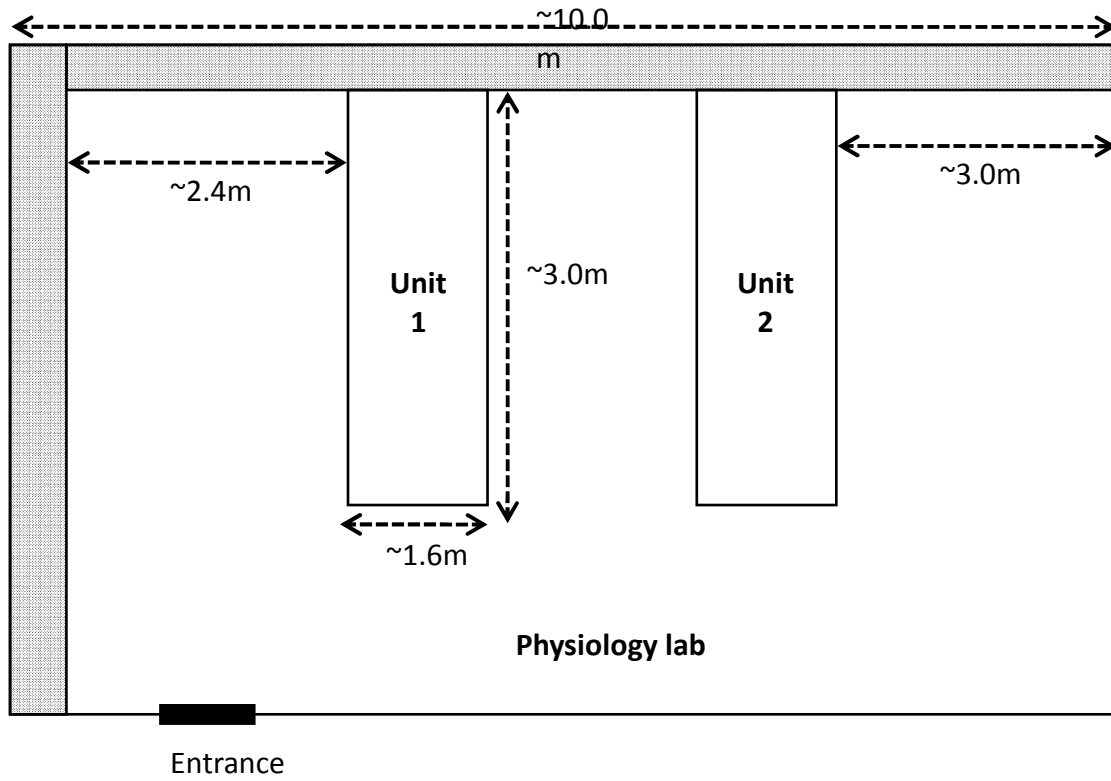

Front view

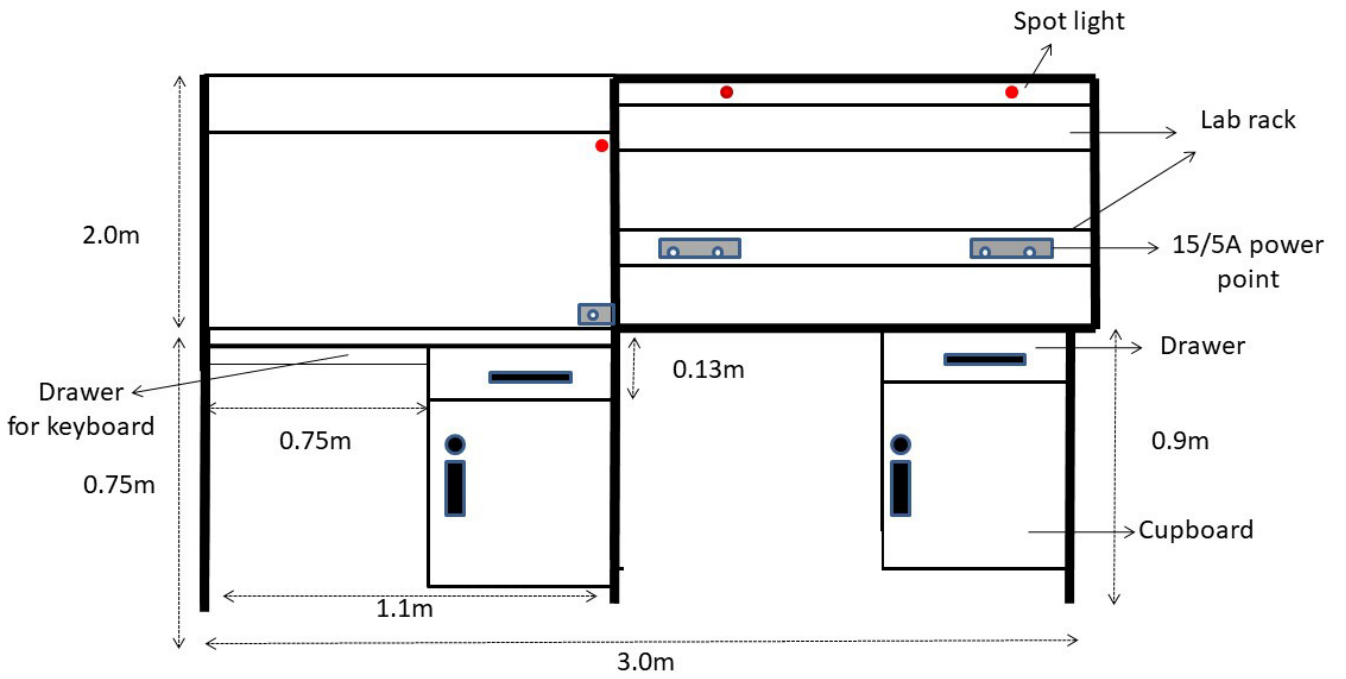

Terms & Conditions for Submission of Tenders.

1. Tenders/Quotations shall be submitted only by online mode through Central Public Procurement Portal at <https://eprocure.gov.in/eprocure/app>.
2. Tender should be submitted Against each item by online mode through Central Public Procurement Portal at <https://eprocure.gov.in/eprocure/app>.
3. **Tenderers/Bidders after submission of their bids online through CPP Portal must submit Physical/Hard Copy of all the submitted/uploaded documents on portal except Financial Bid (BOQ) alongwith Tender Fees and EMD which should reach at ICAR-NRC on Pig, Rani, Guwahati on or before 1.00 P.M, 21.03.2018 failing which their tenders/bids will not be considered and treated cancelled.**
4. Manual/Offline bids will not be accepted under any circumstances from the Bidders/Tenderers who had not submitted their bids online through CPP Portal.
5. Online Tenders must be submitted at CPP portal before **1.00 PM, 21.03.2018**
6. Online Technical Bids will be opened on **1.00 P.M,22.03.2018.**
7. Tenderers/bidders are requested to visit the above website regularly. Any changes/modifications in tender enquiry will be intimated by corrigendum through this website only.
8. The Director,ICAR-NRC on Pig,Rani,Guwahati shall have the right to reject all or any of the offers . Accept one or more than one offer, and assign part of the job.
9. The goods shall be supplied & installed at ICAR-NRC on Pig, Rani,,Guwahati within 30 days of the order by the Institute. The amount quoted in the BOQ should be inclusive of all charges and taxes.
10. Correction or over- writing in the tender documents is not permissible. Every sheet of the Tender document and the terms and conditions should be signed and stamped by the authorized signatory of the firm.
11. All taxes, levies extra, if any should be specifically indicated. Any variation (increase of/decrease) in taxes etc. during the currency of the contract period shall be payable as per the rules in vogue at the point of time.
12. The bidder should not have been Black listed by any Government Department/Organization. **Necessary Certificate/Undertaking should be submitted by the bidder that their firm had never been blacklisted/banned by any Govt. organization in India.**
- 13 The bid should be furnished in two bid system i.e Technical Bid and Financial Bid (BOQ). The bid should contain the following documents as per the term & conditions of the tender document without which tender/bids will be rejected.
 - a. Proof of Registration with the GST, PAN /TAN Copy.
 - b. Proof of income tax Assessment/Return for the last Two years.
 - c. Proof of Annual Turn Over which should not less than 5 Lakhs for the Last Two years.
 - d. Earnest Money in the form of Demand Draft/PBG/FD Drawn in favour of Director-ICAR-NRC on Pig, Rani,Guwahati ,payable at Khanapara have to be deposited along with documents in bid of **Rs.10,000.00** which shall be refunded without interest after finalization of contract. If the firm is exempted from the payment of EMD, copy of NSIC Registration certificate must be submitted.
 - f. Tender fees in the form of Demand Draft Drawn in favour of Director-ICAR-NRC on Pig, Rani,Guwahati ,payable at Khanapara have to be deposited along with documents in bid of Rs.500.00.
 - g. Certificate/undertaking that the firm is never been blacklisted/banned by any Govt. organization in India.
 - h. Client List.
 - i. Experience Certificate
14. **The company can physically inspect the site before participate in the tender.**
15. **All the supplied items must have atleast 05 years warranty from the date of supply/installation.**
16. Mere quoting of lowest rates does not mean that order shall be given to that firm. However the competent authority will decide with the view of approved sample and price quoted.

S/d
(M. Besra)
Administrative Officer